Calculations are performed using daily time steps. The 30-day volume-weighted average for a particular day is calculated using a ‘window’ of time which includes the previous 30 days which had both flow and measurements of radionuclide activity. Therefore, for a location with continuou flow and complete analytical results, 365 (366 in a leap year) 30-day average values are calculated annually. When a negative analytical result (e.g. -0.002 pCi/l) is returned from the lab due to blank correction, then a value of 0.0 pCi/l is used for calculation purposes.

ıge for a
/s which
ı continuous
re
ɔm the lab

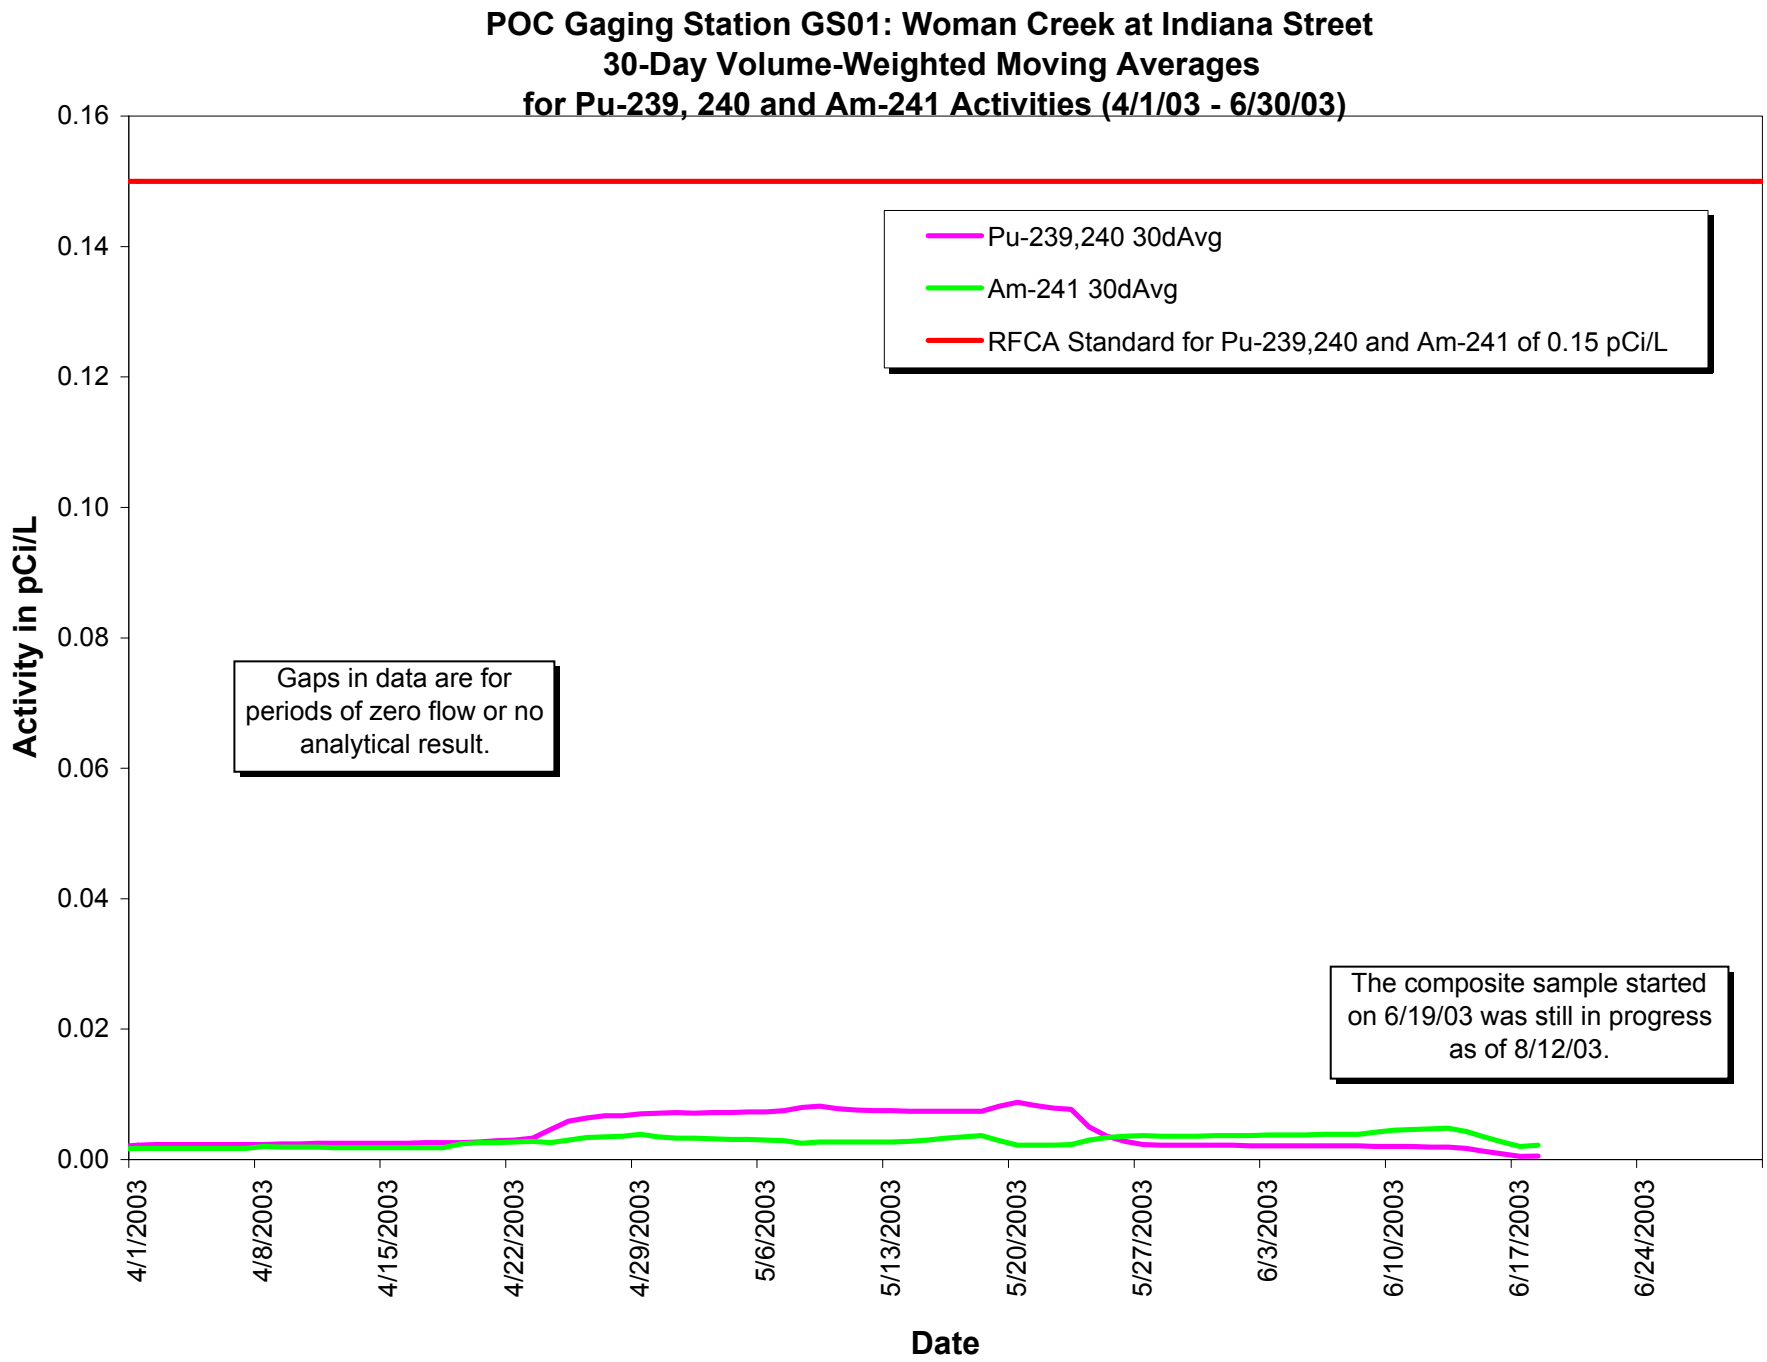

Print Date: 9/4/2003

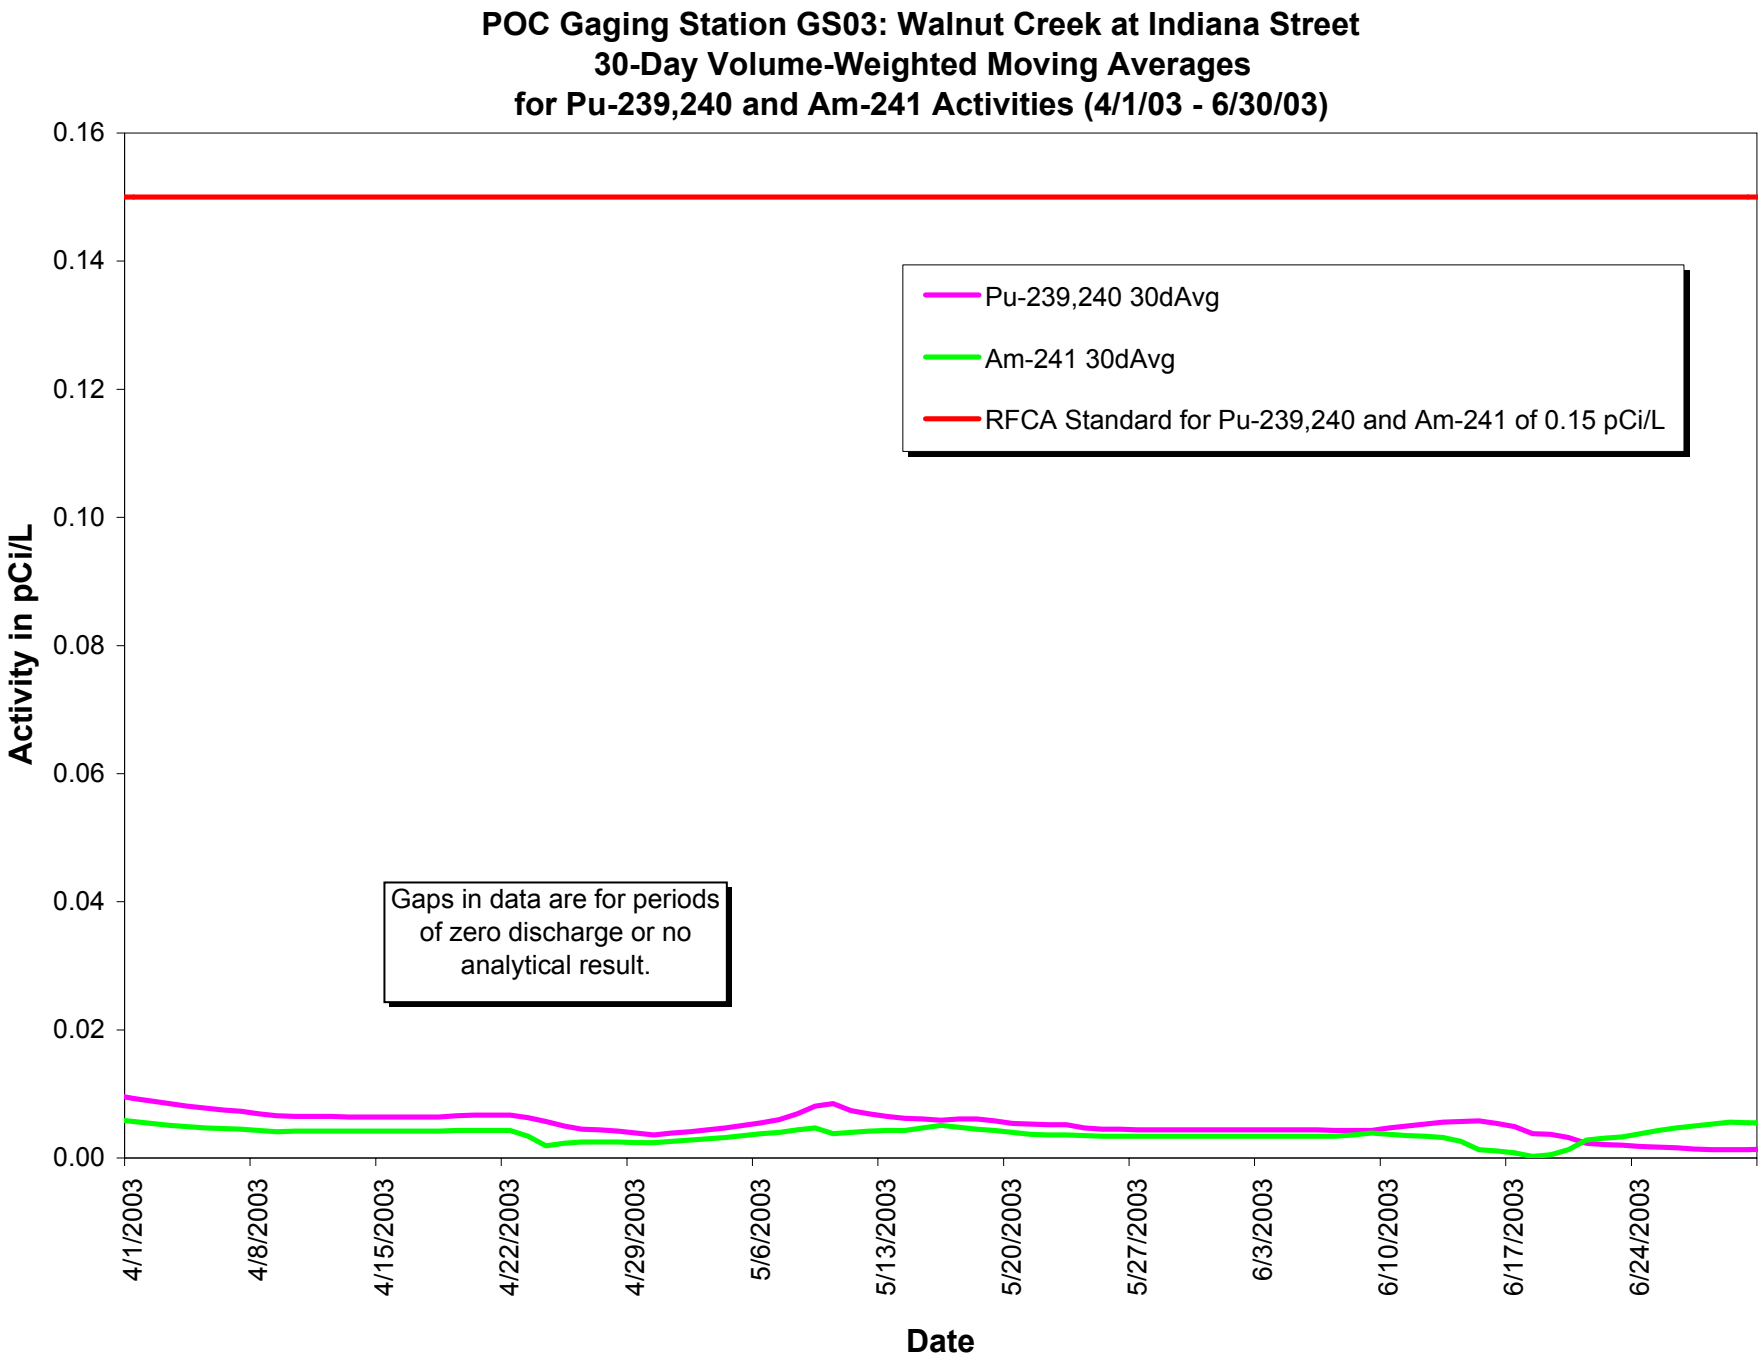

Print Date: 9/4/2003

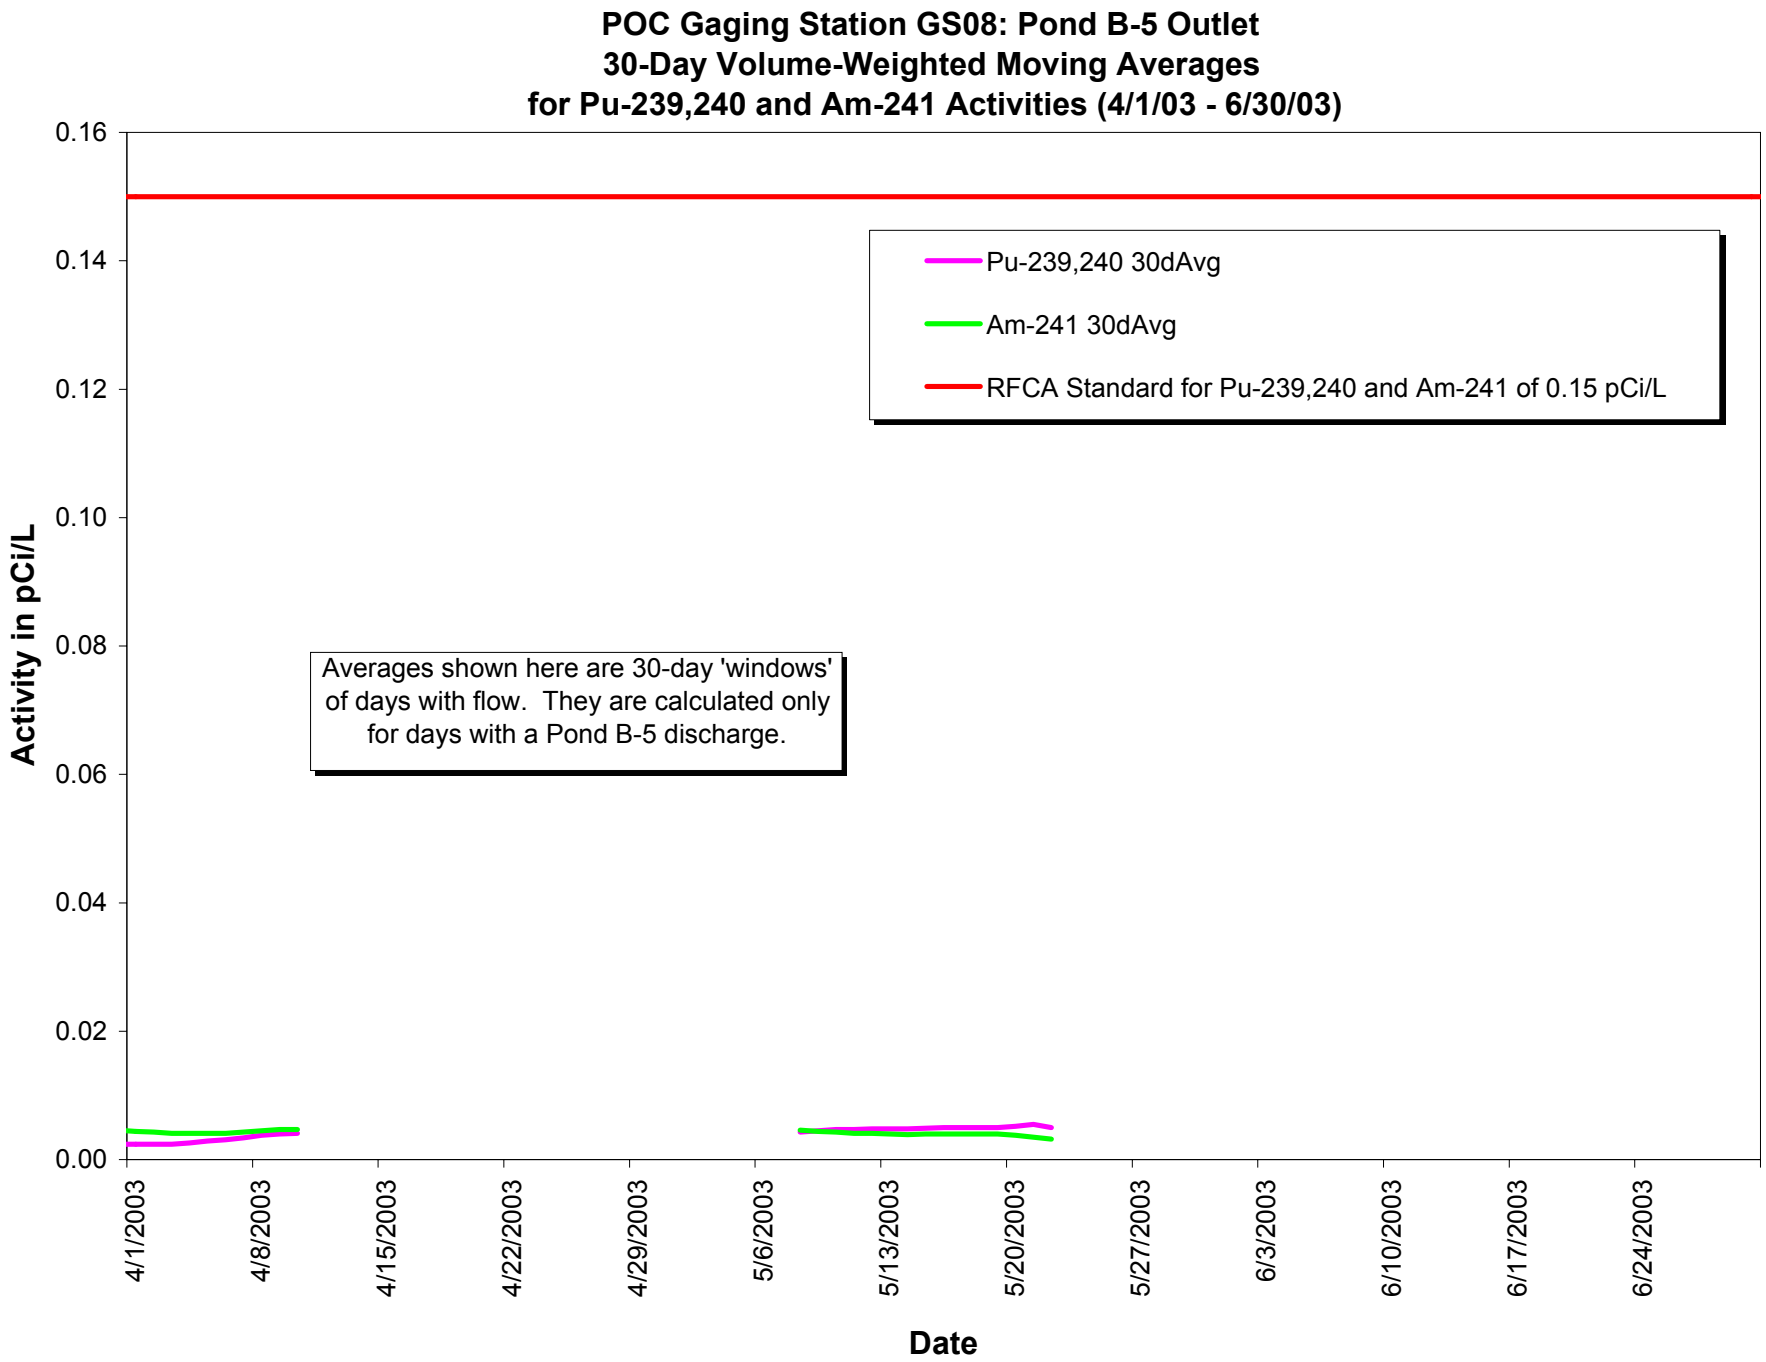

Print Date: 9/4/2003

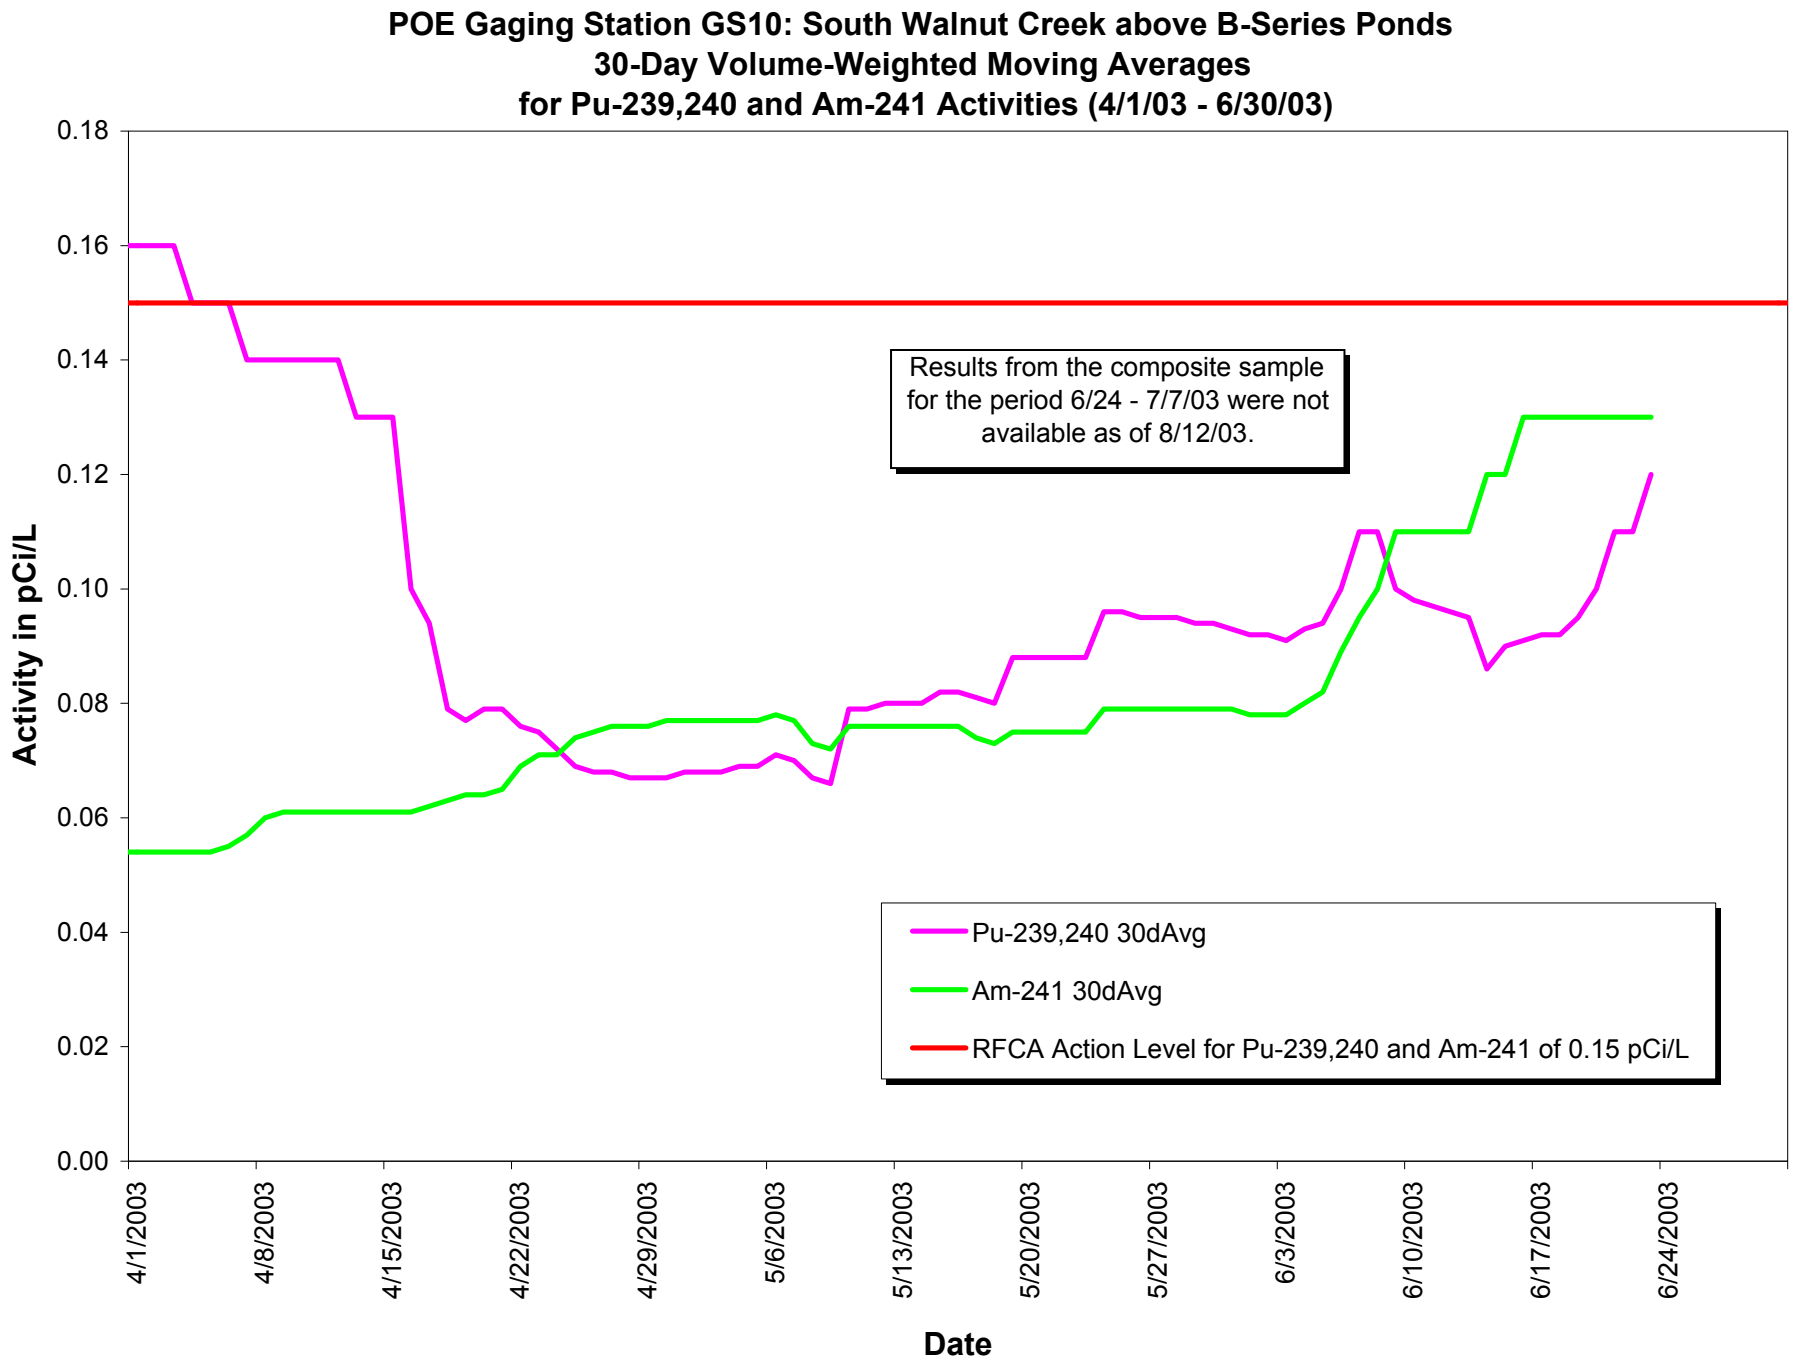

Print Date: 9/4/2003

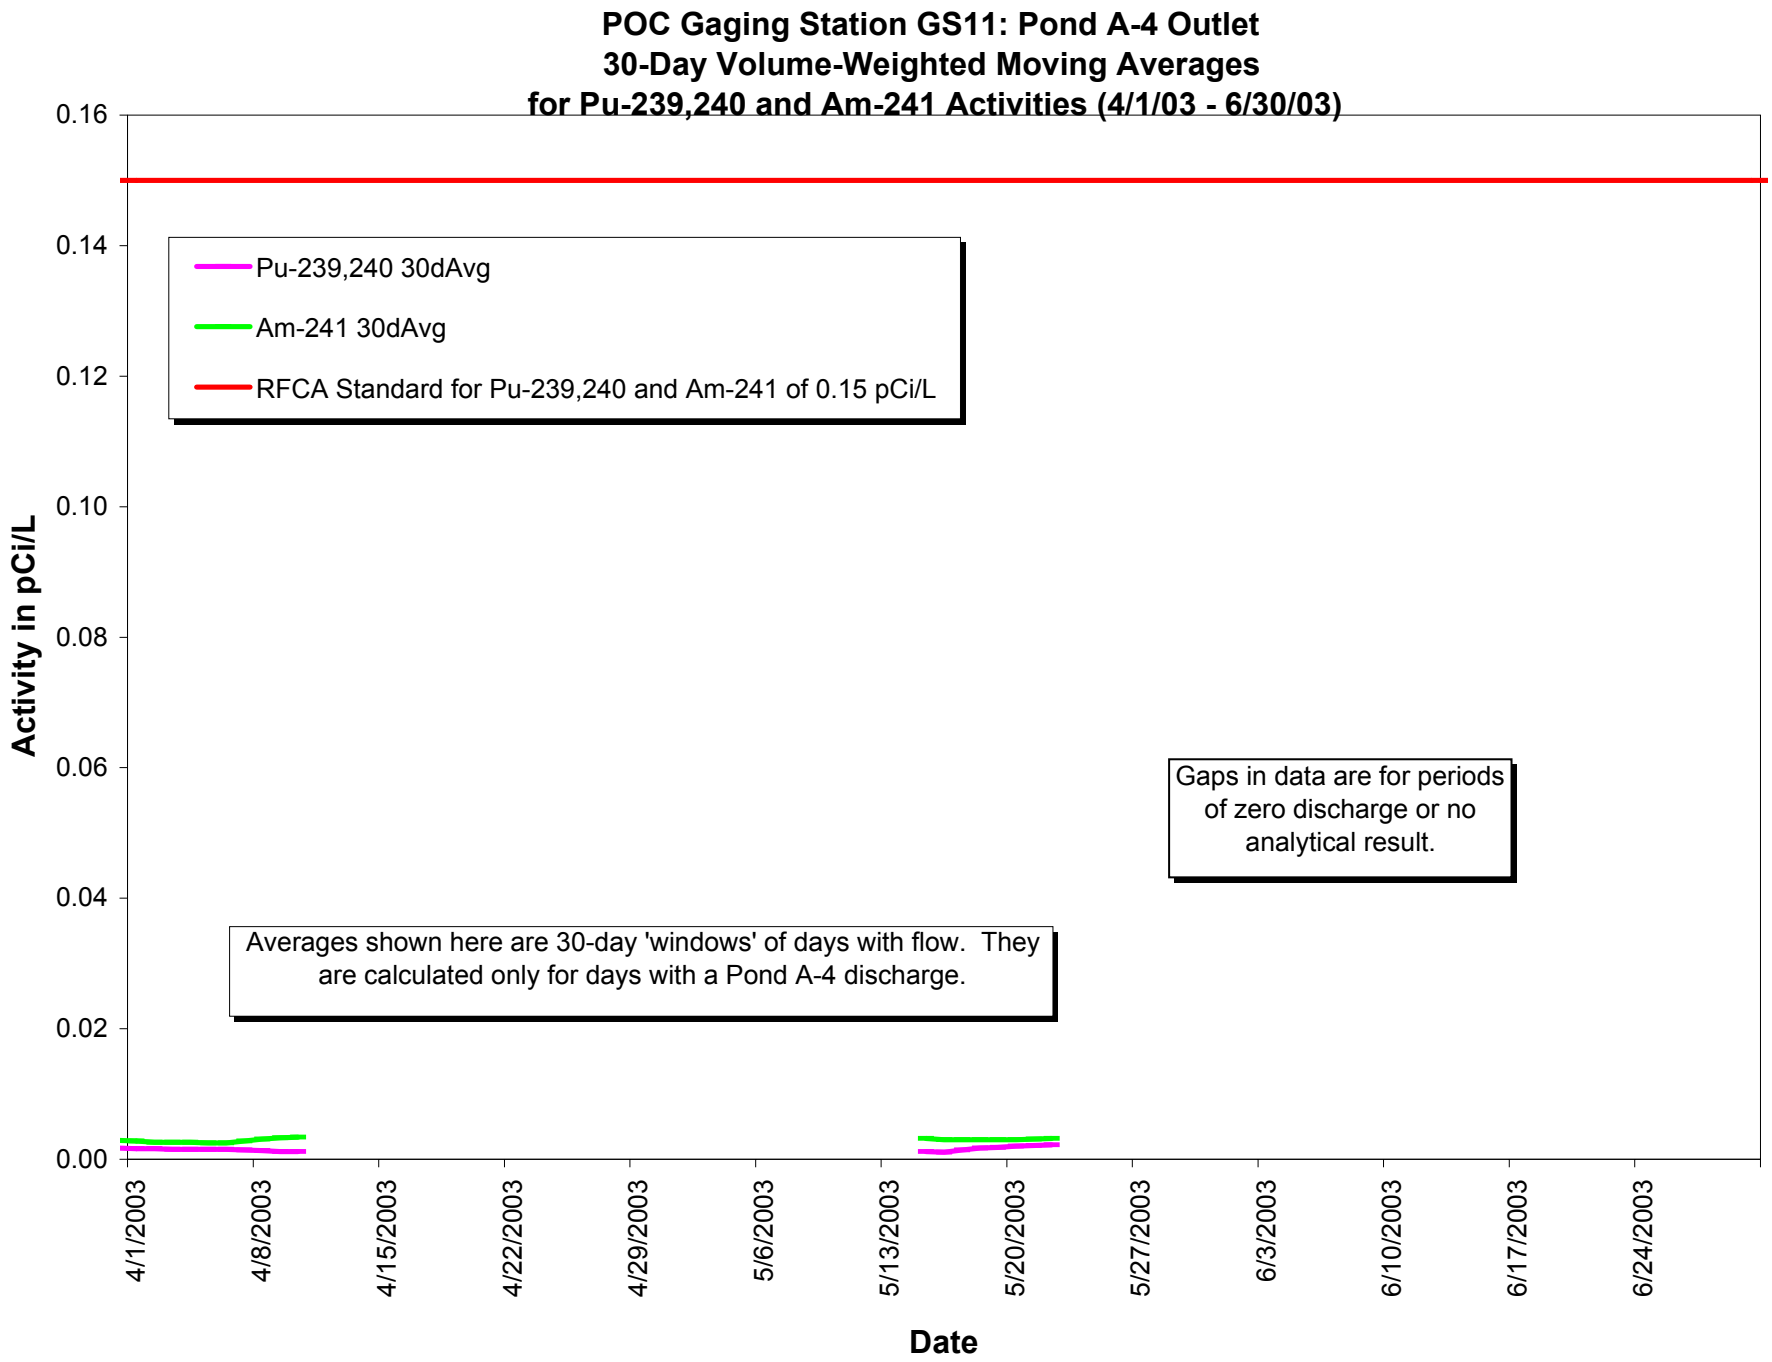

Print Date: 9/4/2003

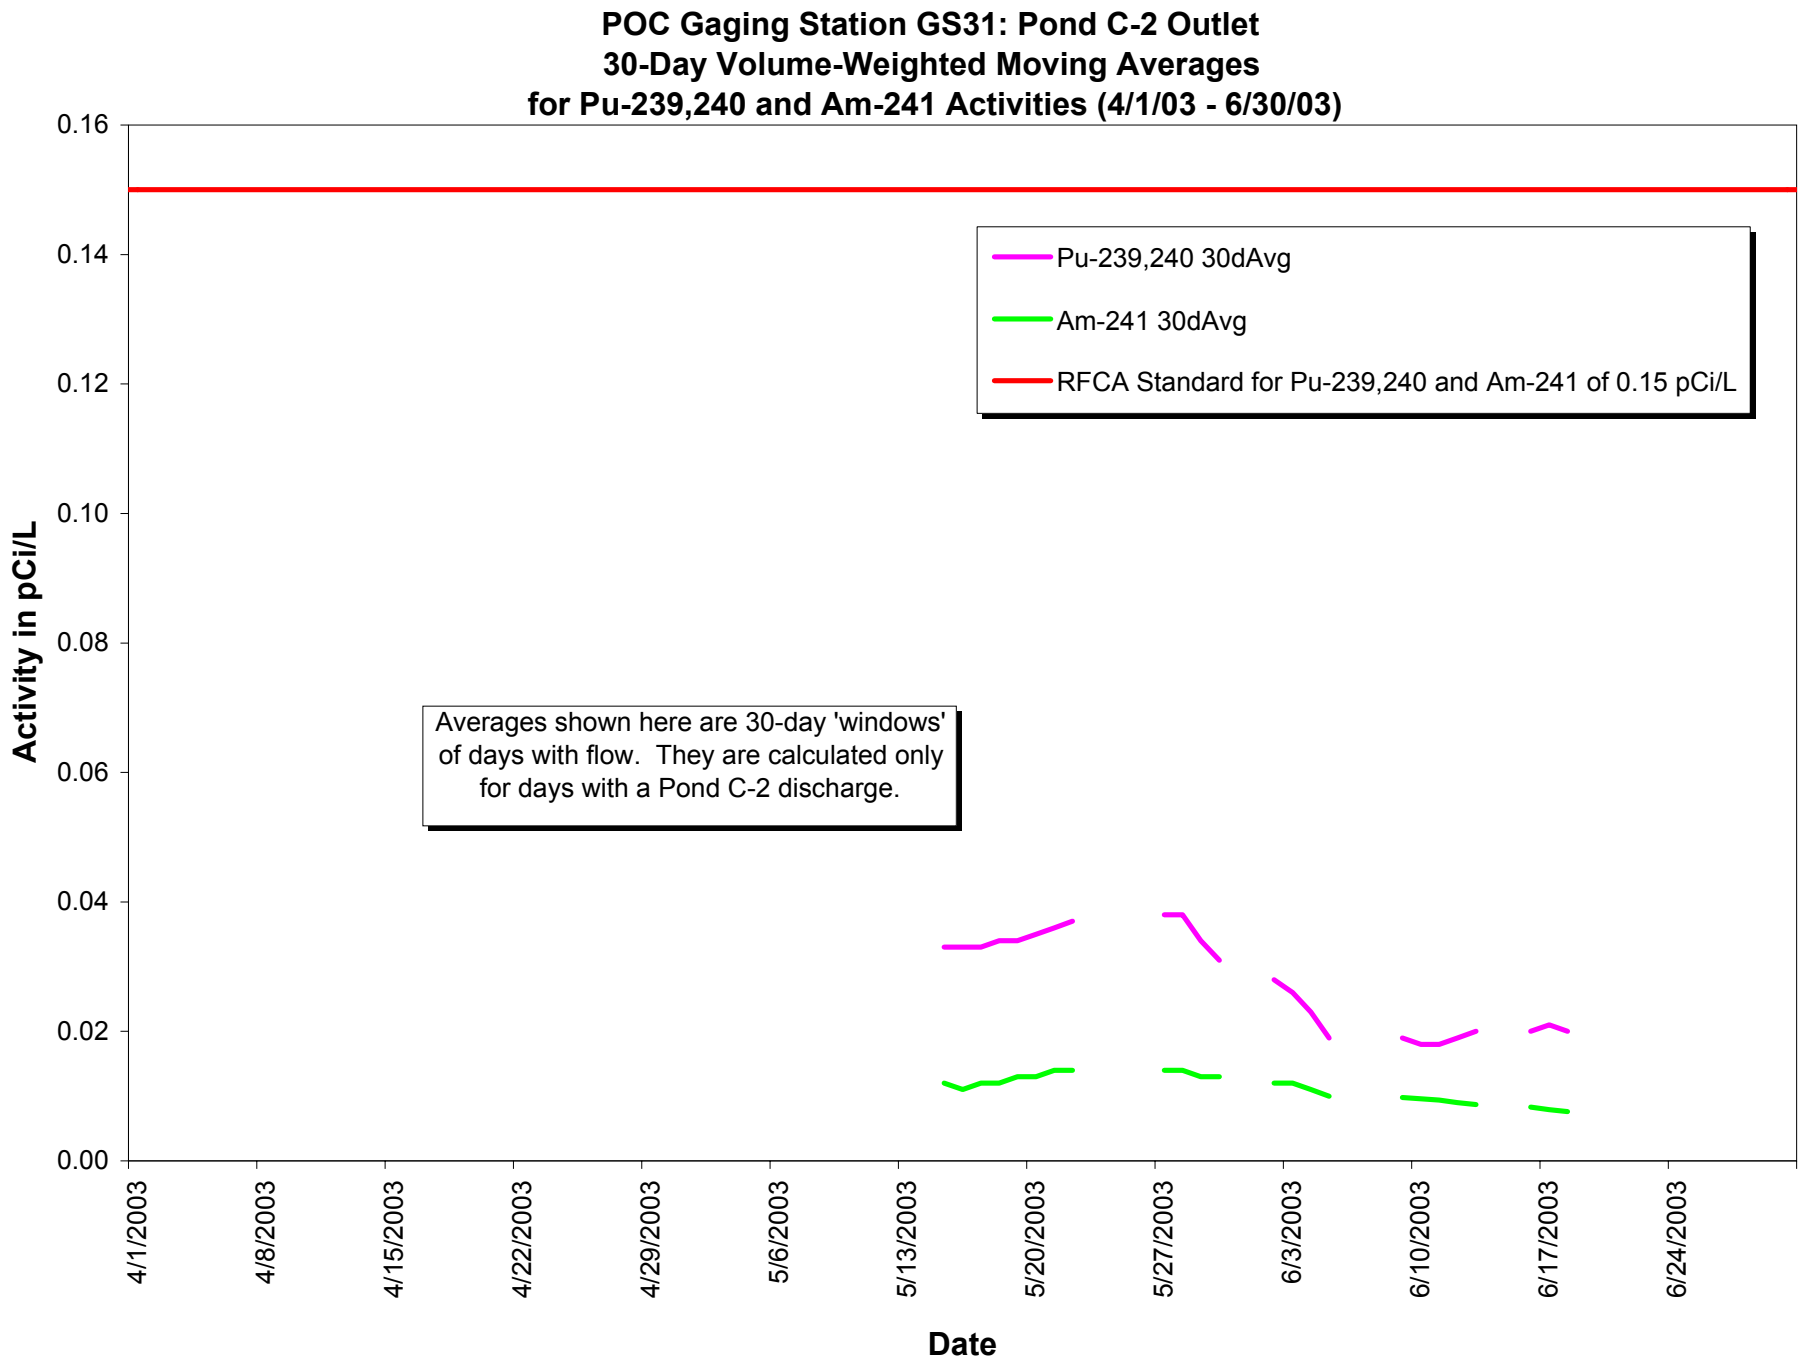

Print Date: 9/4/2003

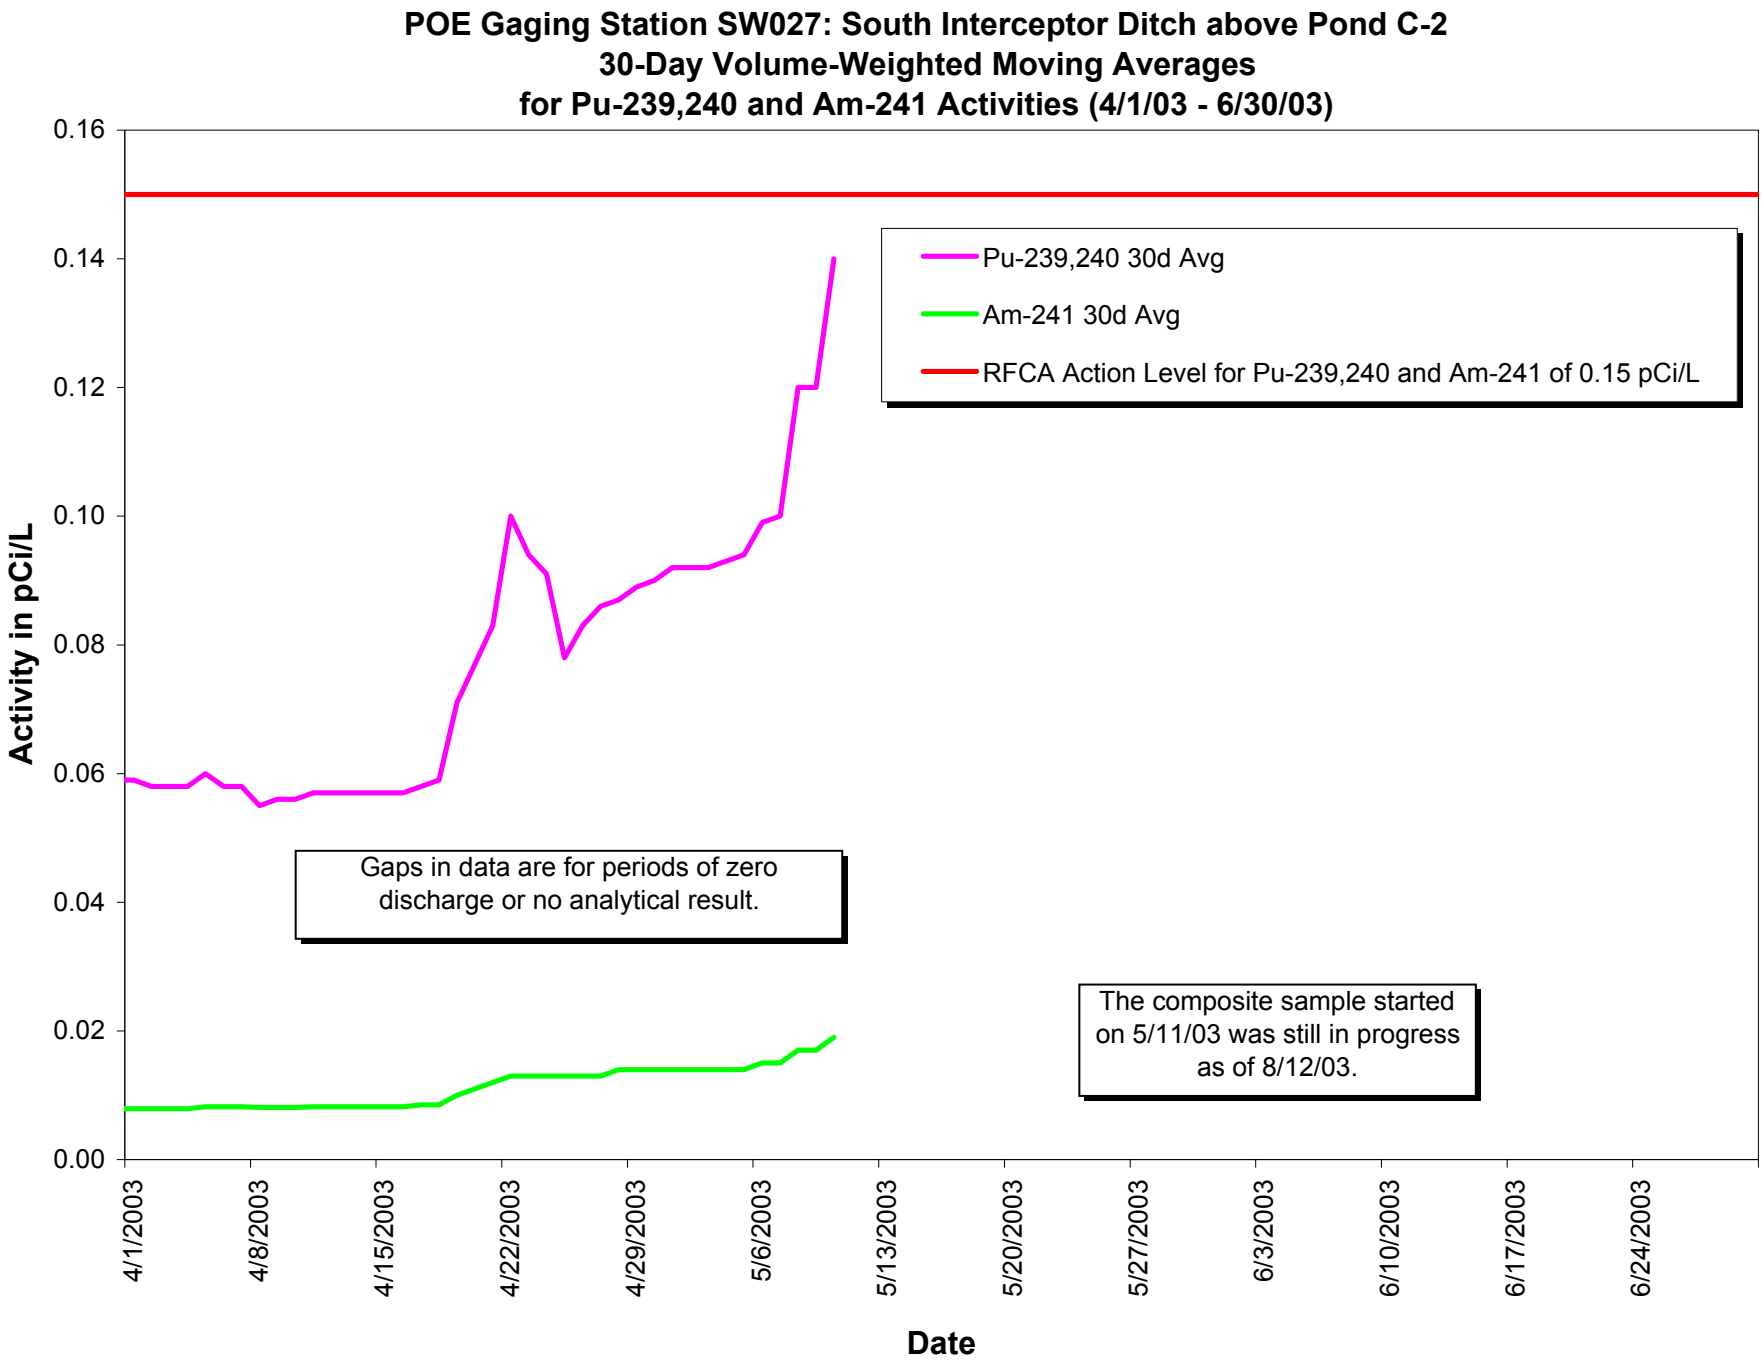

Print Date: 9/4/2003

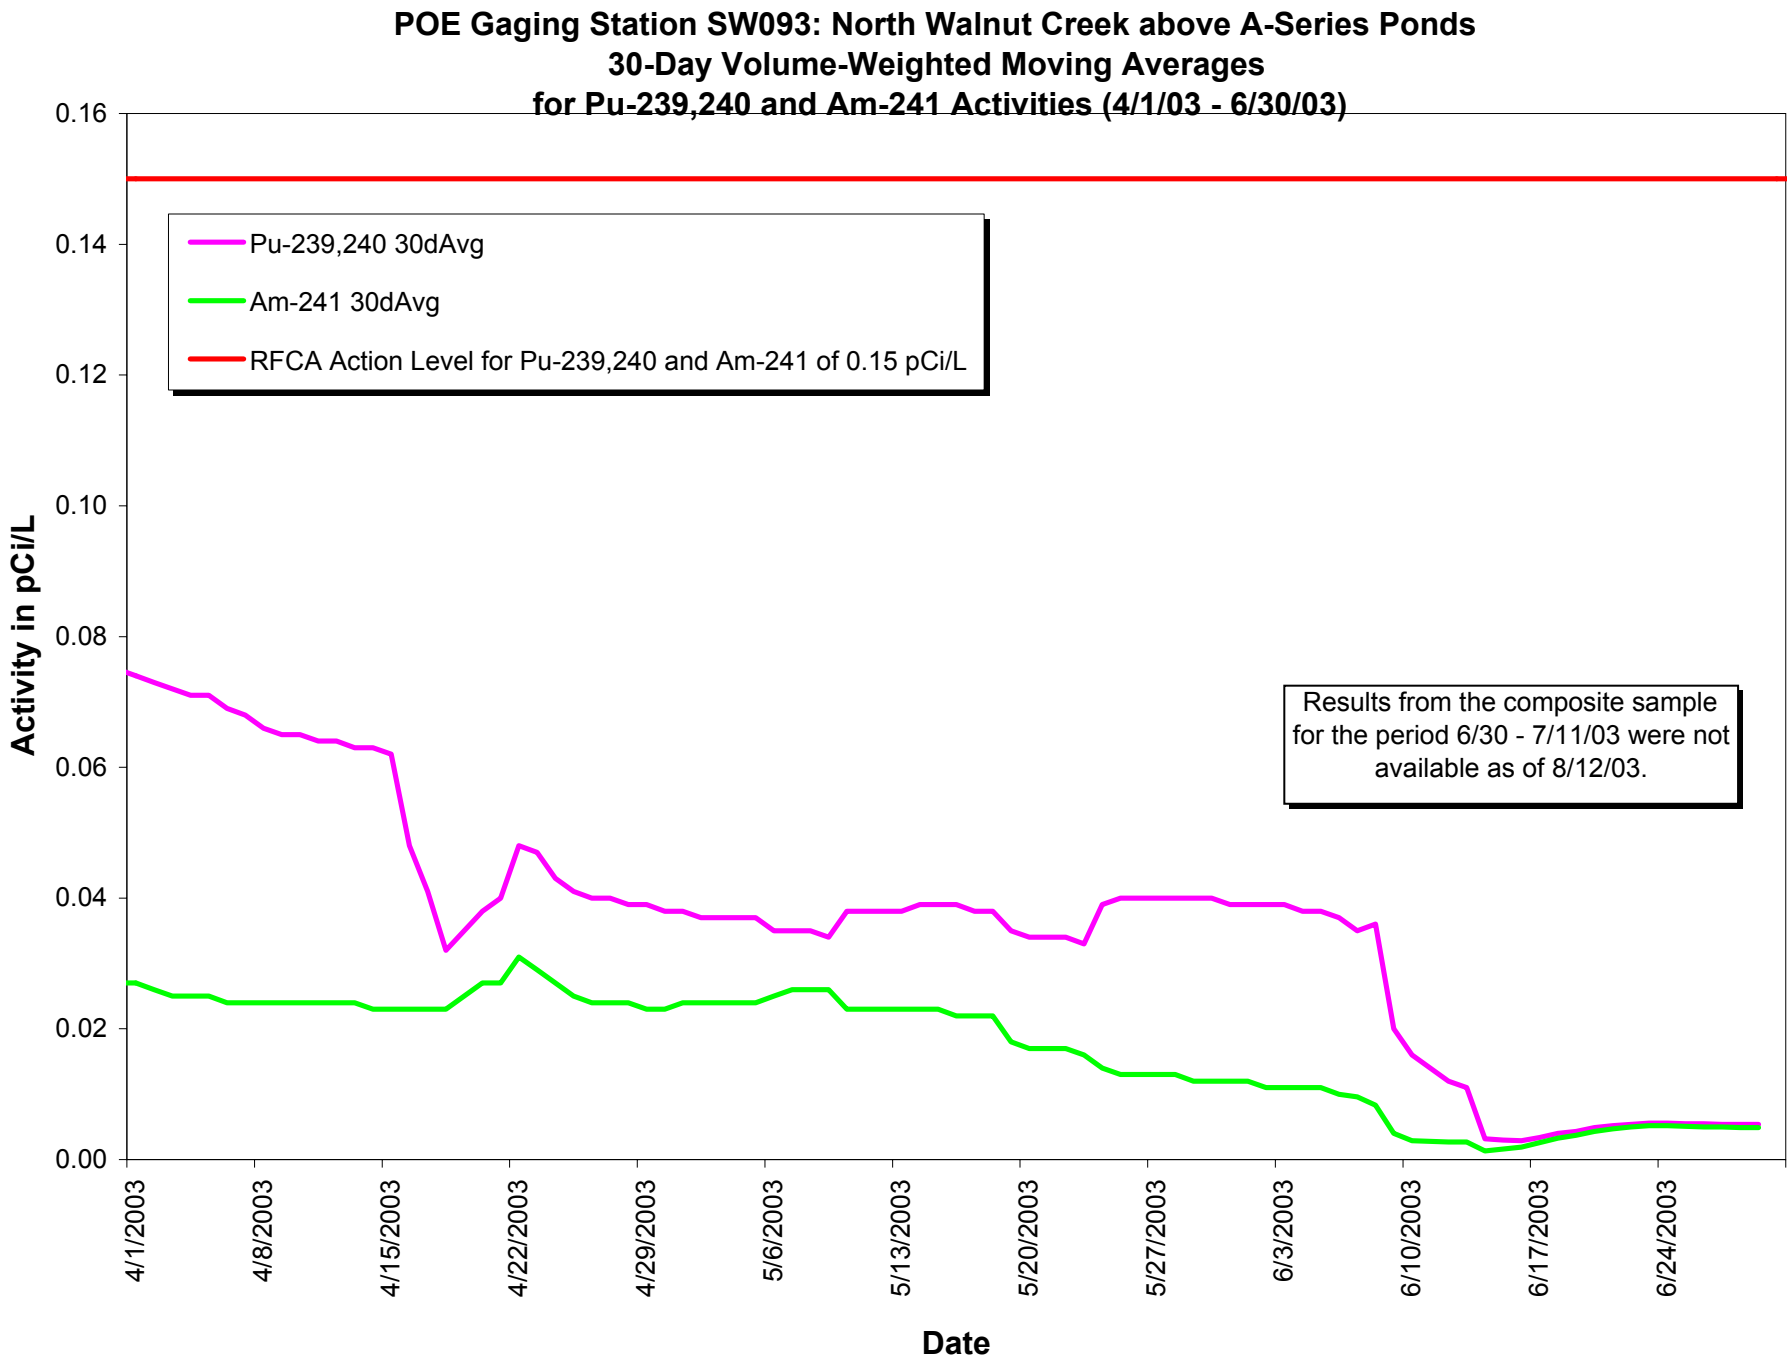

Print Date: 9/4/2003

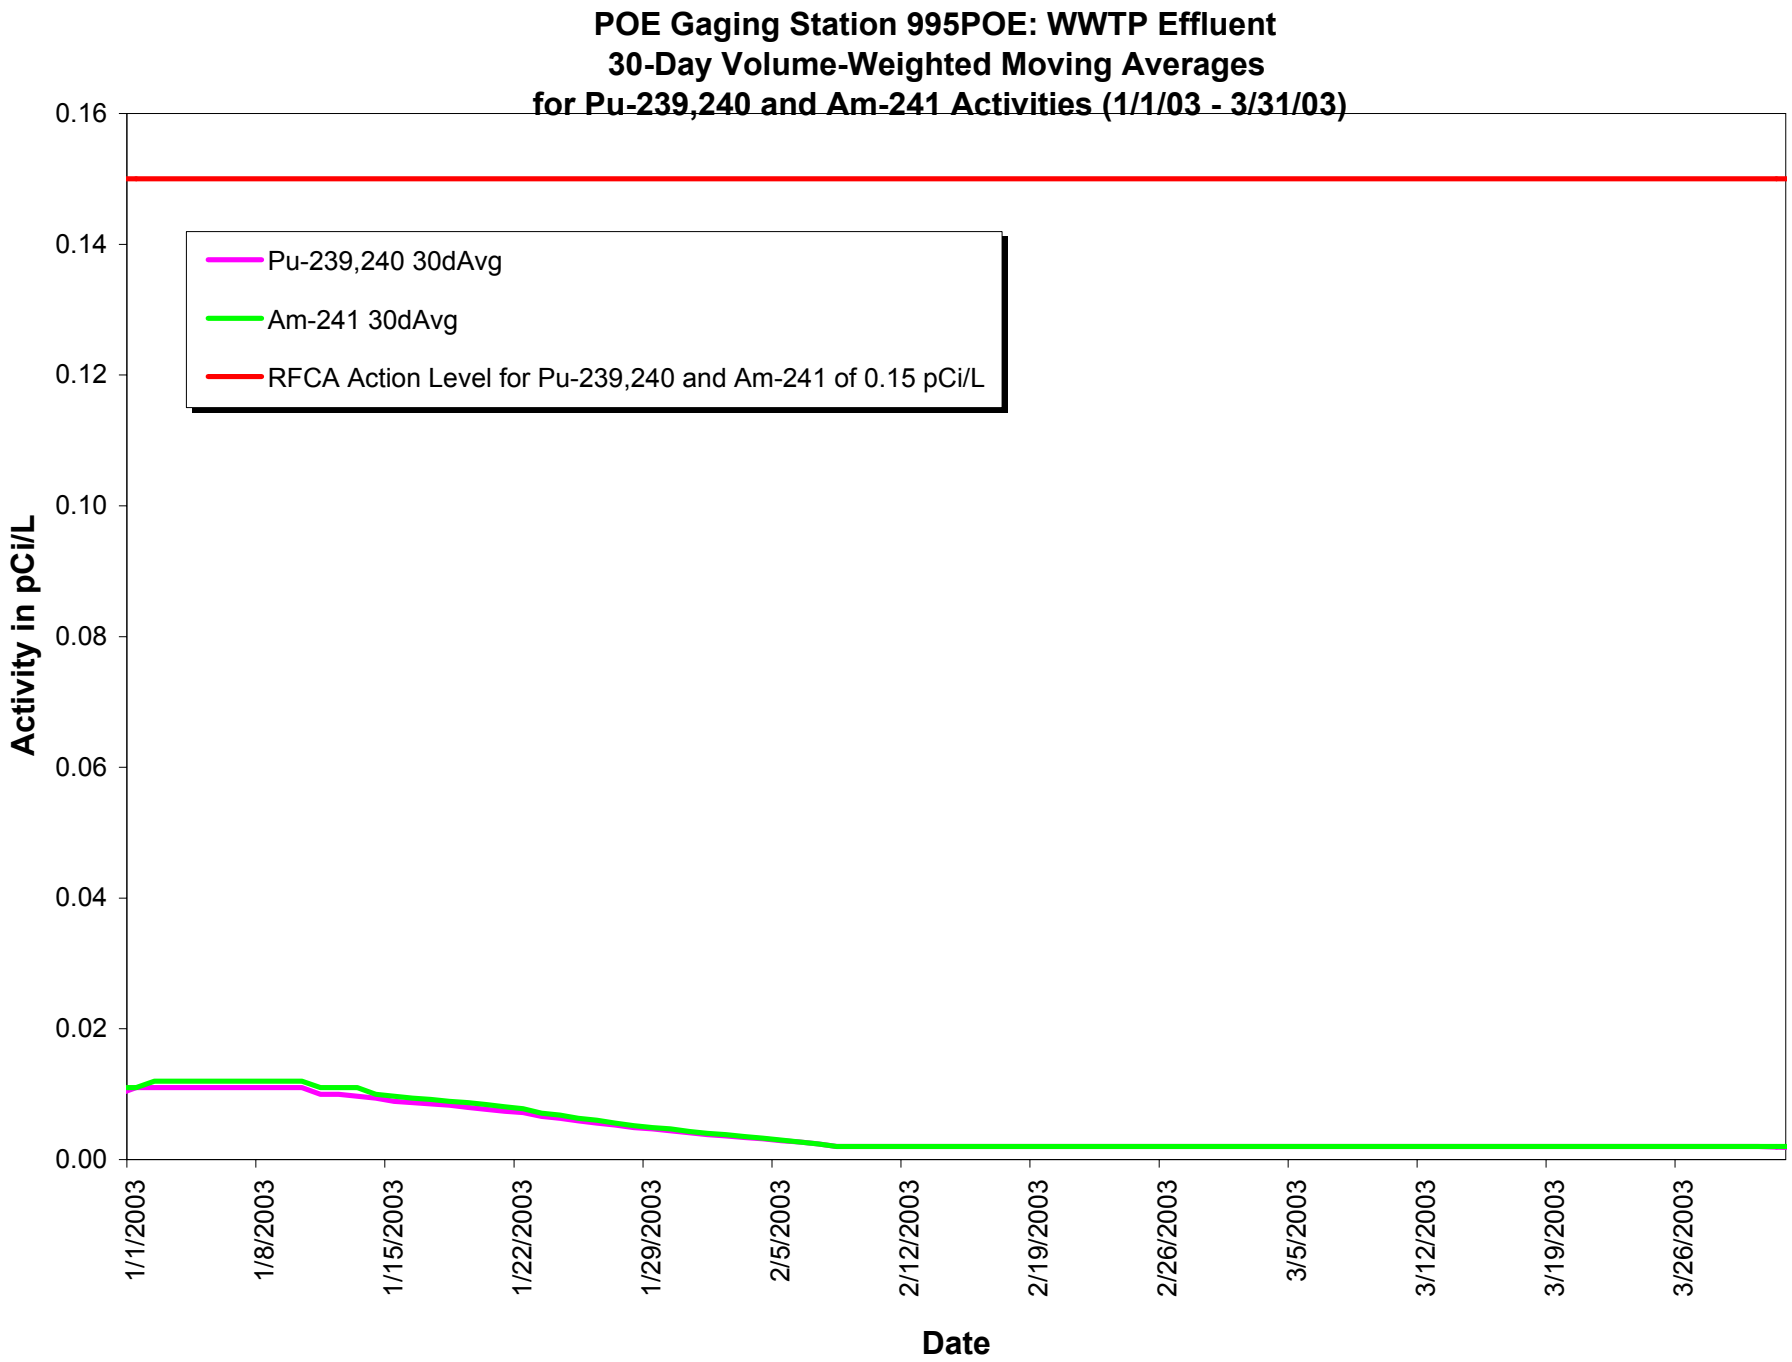

Print Date: 9/4/2003

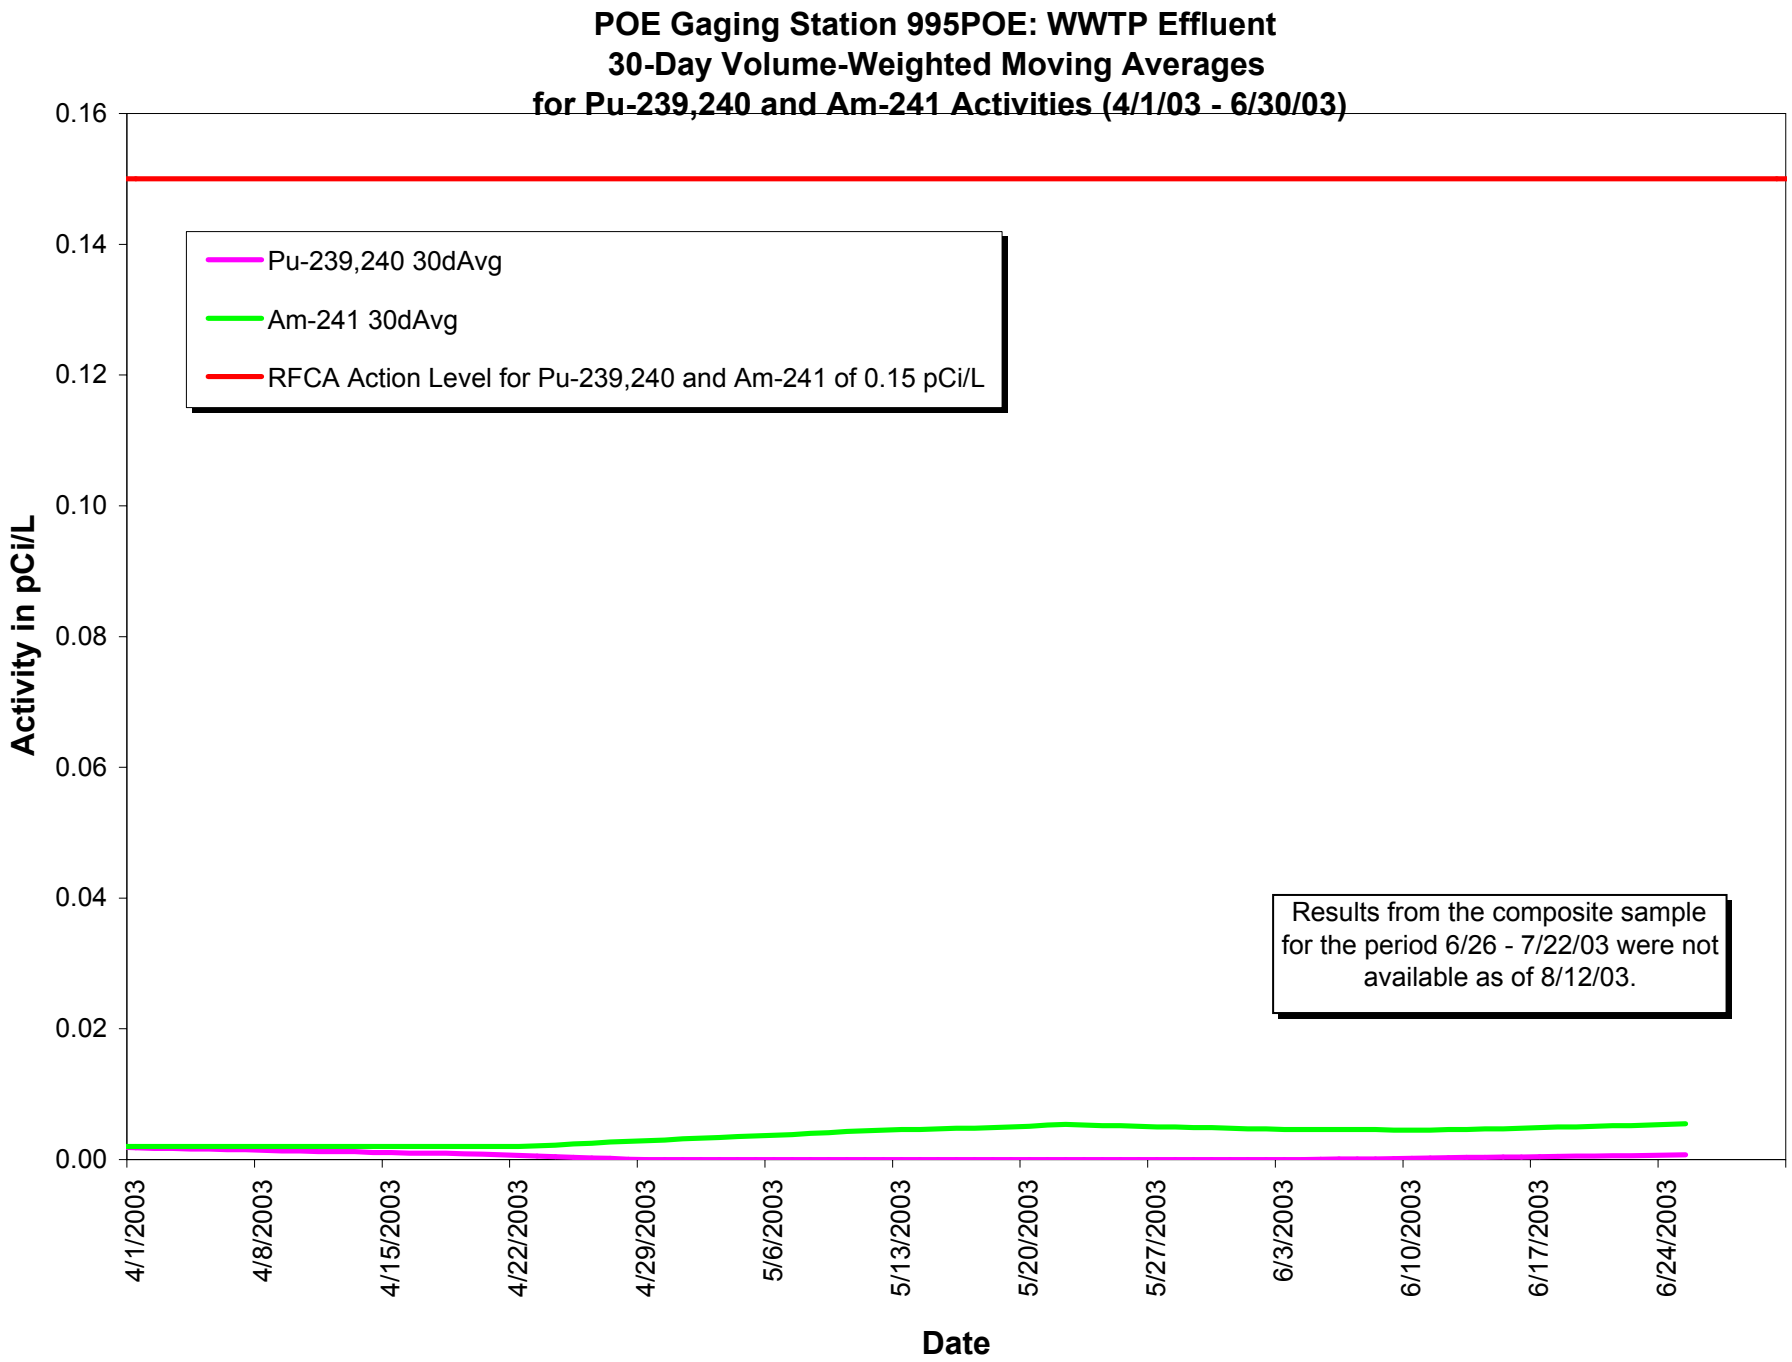

Print Date: 9/4/2003